

RA# _____
(eMail service@ika.net prior to shipping)



designed for scientists

Decontamination Certificate

/// IKA Equipment

Please take into consideration that, due to safety-related reasons, we will not be able to process your repair without this completed Decontamination Certificate.

Customer's Shipping Address

Company	Country
Contact person	Phone
Dept. / Lab. No.	E-mail
Street	City / State / Zip Code

For International Customers: Please provide Broker Agent's information and contact details, and a shipping account number or a method of payment to cover the shipping fees to return the repaired unit back to you.

Instrument data

Instrument Type (e.g. EUROSTAR digital)	Serial Number	Reason for return

Substances used with the device:

Legally binding declaration

1. The IKA-equipment resp. part has been carefully cleaned and freed from remaining material / substances before returning to IKA.
2. As far as this was possible, we herewith declare, that the remaining material / substances have no harmful or risky influence on the IKA personnel handling the instrument.
3. A further cleaning by IKA with usual cleaning agents is harmless and cannot cause any harmful consequence (e.g. chemical reactions).
4. The declaration concerning items 2 and 3 are given in account to the best of our knowledge and belief and under consideration of our obligation to care.
5. A second signature is given by the person responsible for the condition of the goods immediately prior to return delivery.
6. The client confirms, that the returned goods do not represent any danger by bacteriological, virological, chemical or radioactive contamination.
7. The undersigned is authorized to give such declaration in the name of the represented company.
8. The client is aware of the fact that he / she is liable towards the consignee for any damages caused by incomplete or incorrect information.
9. The warranty does not cover any shipping charges.

Company Stamp

Date

Signature


Second signature



designed for scientists

Packaging Instructions


/// Non-freighted Laboratory / Analytical Equipment

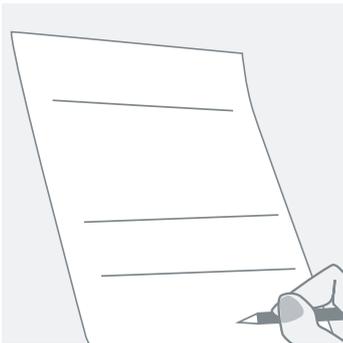


Please fill out the Decontamination Certificate.



Pack the instrument, if possible, in the original carton, and then into a shipping box.

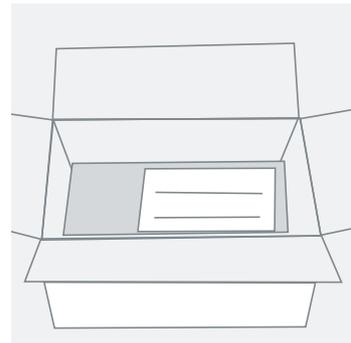

Please package the instrument safely. Place completed Decontamination Certificate in the box. Cushion with either original packaging or suitable materials.

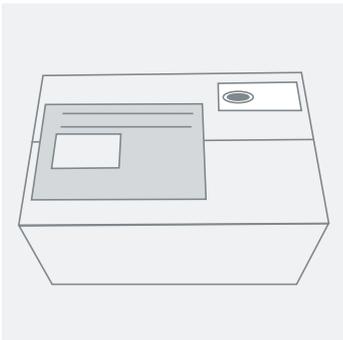

Put the shipping documents in a mailing pouch. Attach the "No Danger" sticker to the shipping box so that it is clearly visible.

Please make sure the RA# is clearly written on the outside of the box.



The instrument in this package will not cause any danger due to bacteriological, virological, chemical or radioactive contamination.


Das in diesem Paket enthaltene Gerät ist frei von jeglichen bakteriologischen, virologischen, chemischen oder radiaktiven Verunreinigungen.

Decontamination Certificate attached


Unbedenklichkeitsbescheinigung liegt bei

Packaging Instructions


/// Freight Laboratory / Analytical Equipment

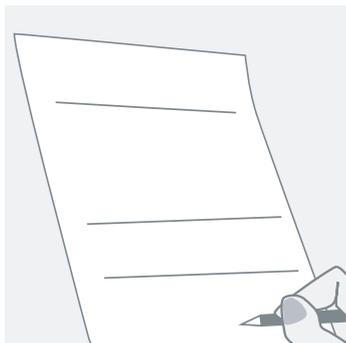

Please fill out the Decontamination Certificate.

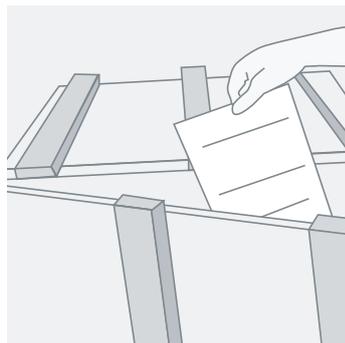

Pack the instrument into a cardboard box or a wooden box, depending on the size of the machine, secure it to a pallet and include a copy of the Decontamination Certificate.

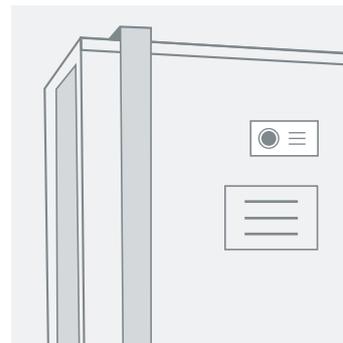

Put the delivery note and the Decontamination Certificate into a protective bag and fix it together with the sticker "No Danger" on the outside of the package where it can easily be seen.

Please make sure the RA# is clearly written on the outside of the box.

LAB & ANALYTICAL UNITS THAT MUST BE PALLETIZED FOR SHIPMENT:

Calorimeters: C 1, C 200, C 2000, C 5000, C 6000
CBC / HBC / HRC
HS/KS 501 digital Shaker
IC basic / control
IKA Dry Oven
KS 3000 Shaker
KS 4000 Shaker
LR 2 Lab Reactor
LR 1000 Lab Reactor
Maxi MR 1 digital Magnetic Stirrer
MVP 10
Photo Bioreactor
RC 2 Chiller
RV 3 Rotary Evaporator
RV 8 Rotary Evaporator
RV 10 Rotary Evaporator
RW 47 Mixer
T 65 Disperser
Vacstar control



Die in dieser Verpackung enthaltene Maschine wurde vor Versand gereinigt und ist frei von jeglichen bakteriologischen, virologischen, chemischen oder radioaktiven Verunreinigungen.

The machine in this package has been cleaned before dispatch and does not mean any danger due to bacteriological, virological, chemical or radioactive contamination.

Decontamination Certificate attached

Unbedenklichkeitsbescheinigung liegt bei